




Quality and Stability Report for Glutathione


Product Name	GSH	Manufacture Date	June 1, 2025
Batch No#	N/A	Analysis Date	June 8, 2025
Quantity	1 vial	Expire Date	One Year

Tested Item	Specification	Results
Appearance	Colorless	Complies
Odor	Odorless	Complies
Fluid Clarity	Clear Solution	Complies
pH value	pH=4.0	Complies
Heavy Metals	Test	Complies
Arsenic	Test	Complies
Lead	Test	Complies
Mercury	Test	Complies

Microbie Test		
Total Plate Count	2 plate for 1ml of sample each plate	Complies
Yeast & Mold	Negative (Potate LB Plates)	Complies
Bacteria	Negative (Potate LB Plates)	Complies
Endotoxin Level	<0.01 EU/ml	Complies

Conclusion	The QC data shows no bacterial or fungal contamination in sample. The detailed culture is shown below.
-------------------	---

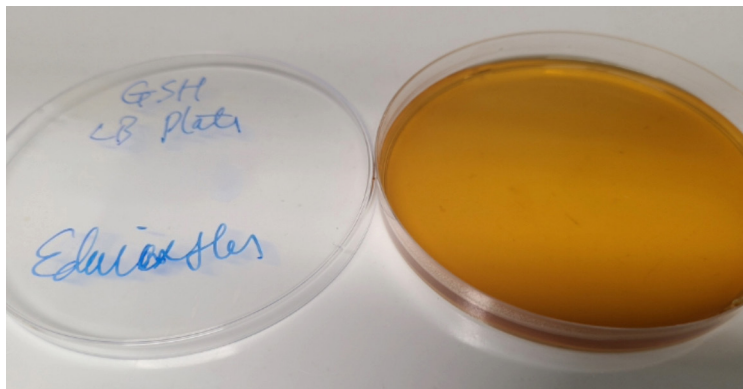



QC Scientist	Edwin Hu, PhD	Report Date	8-June-25
Signature	<i>Edwin Hu</i>	Date	<i>8-June-25</i>